



NE 52-QQ57 HNMR Analysis, Solvent:CDCl3


www.medkoo.com sales@medkoo.com

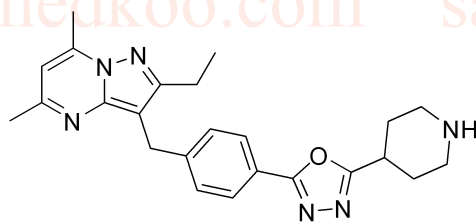

MedKoo Cat#: 555805
 Name: NE 52-QQ57
 CAS#: 1401728-56-0
 Lot#: T20D08P12
 Chemical Formula: C₂₄H₂₈N₆O
 Exact Mass: 416.2325
 Molecular Weight: 416.53

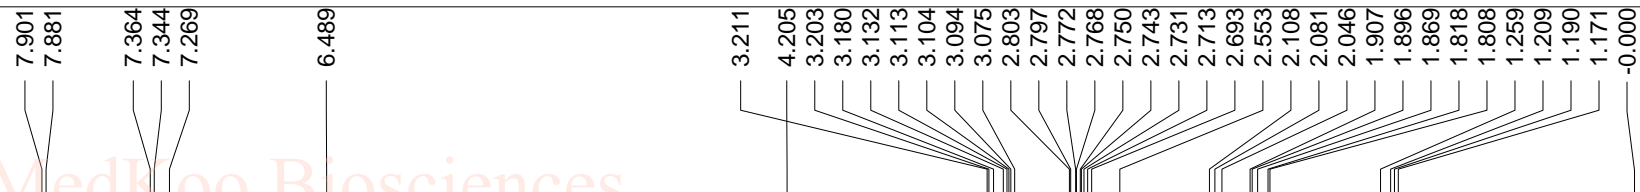

MedKoo Biosciences
 Product Quality Control Data
 www.medkoo.com sales@medkoo.com


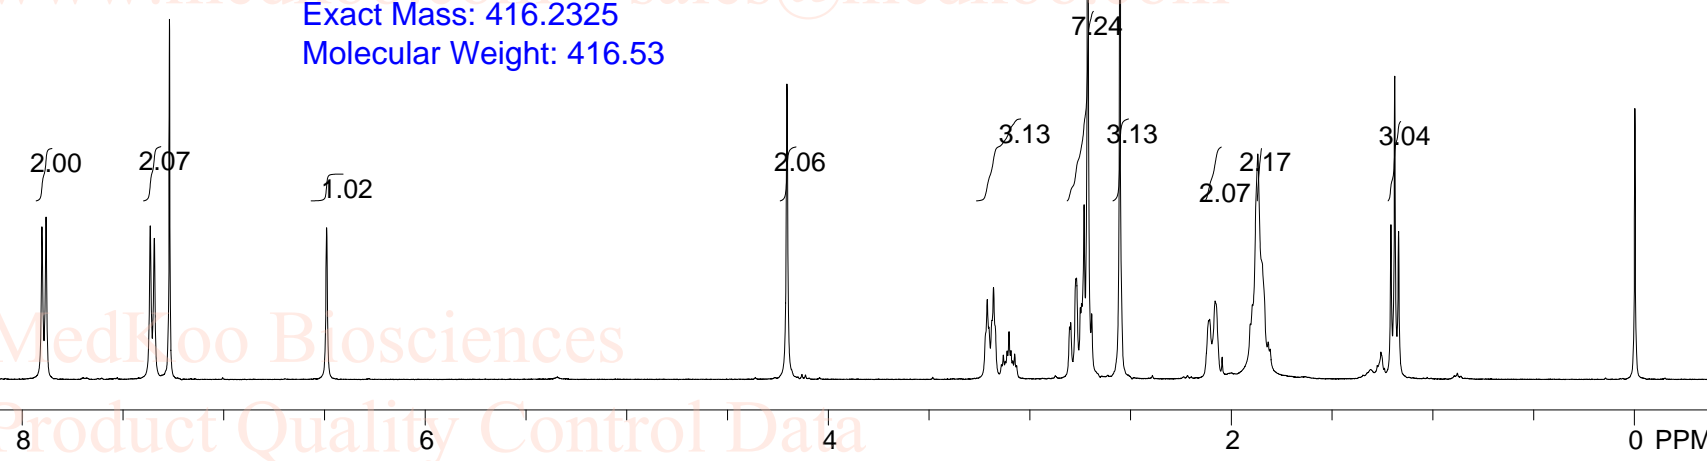


MedKoo Biosciences
 Product Quality Control Data
 www.medkoo.com sales@medkoo.com

NMRB003, CDCl ₃ .		SW1: 8224		OF1: 2467.6		PTS1d: 32768	
F1: 400.232	F2: 1.000	EX: zg30	PD: 1.00 sec	www.medkoo.com	LB: 0.0	sales@medkoo.com	Nuts - \$pdata

NE 52-QQ57 HPLC Analysis

Sample Name : NE52-QQ57 **Location** : P1-E-05
Acq. Operator : **Inj** : 1
Spec. Reported : MS Integration **Inj Volume** : 0.7 ul
Acq. Method : D:\METHODS\1-POS-15MIN.M
Analysis Method : D:\METHODS\1-POS-15MIN.M
Sample Info : Easy-Access Method: '1-POS-15MIN.M'
Method Info : **Mobile Phase**: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5%B increase to 95%B within 8.0 min, 95%B for 7.0 min.
Flow Rate: 1.0ml/min
Column: Sunfire C18, 4.6*150mm, 3.5um
Column Temperature: 40 C
Detection: UV(214,4nm) and MS(ESI, Pos mode, 110 to 1500 amu)

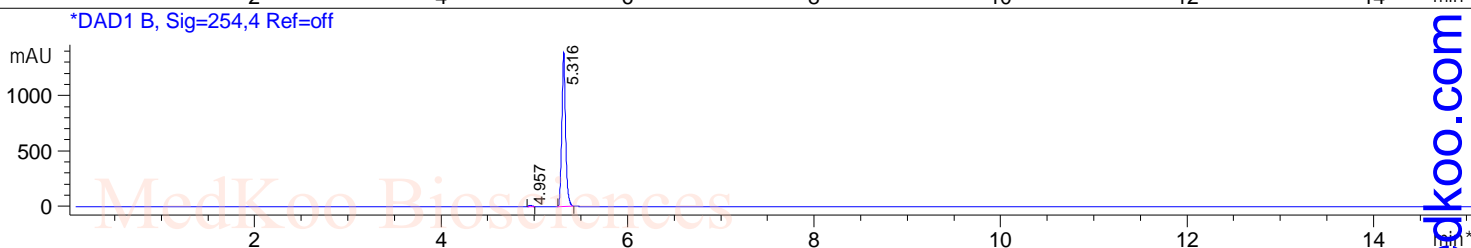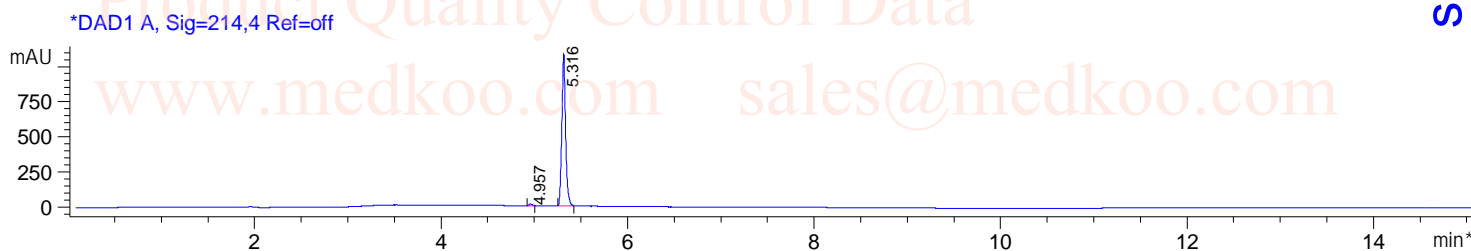


Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
4.96	0.03	26.83	14.33	0.88
5.32	0.04	3039.07	1080.84	99.12

Integration Results for DAD1 B, Sig=254,4 Ref=off




RetTim	Width	Area	Height	Area%
4.96	0.03	21.63	11.84	0.55
5.32	0.04	3898.66	1394.49	99.45

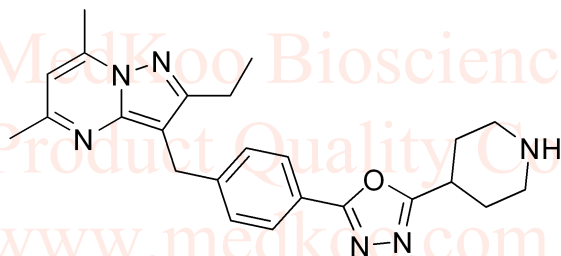

MedKoo Cat#: 555805
Name: NE 52-QQ57
CAS#: 1401728-56-0
Lot#: T20D08P12
Chemical Formula: C₂₄H₂₈N₆O
Exact Mass: 416.2325
Molecular Weight: 416.53


NE 52-QQ57 LC/MS Analysis

Sample Name : NE52-QQ57 Location : P2-B-08
Acq. Operator : System Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\METHODS\1-POS-3MIN.M
Analysis Method : D:\METHODS\1-POS-3MIN.M
Sample Info : Easy-Access Method: '1-POS-3MIN.M'
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5%B increase to 95%B within 1.3 min, 95%B for 1.7 min.
Flow Rate: 2.0ml/min
Column: Sunfire C18, 4.6*50mm, 3.5um
Column Temperature: 50 C
Detection: UV(214,4nm) and MS(ESI, Pos mode, 110 to 1000 amu)

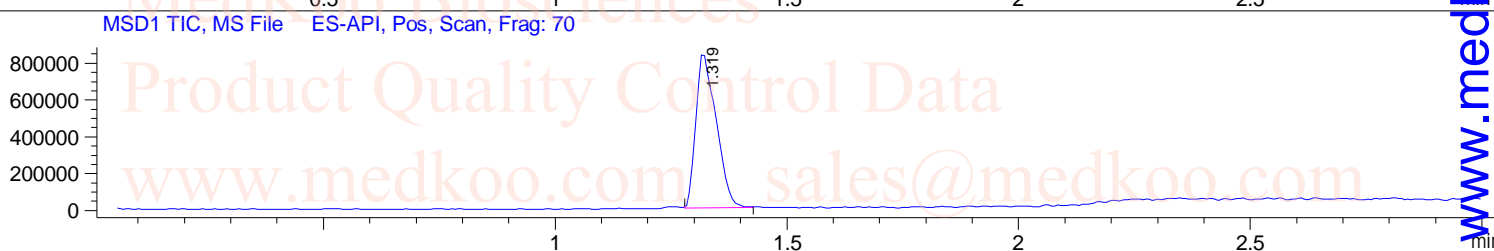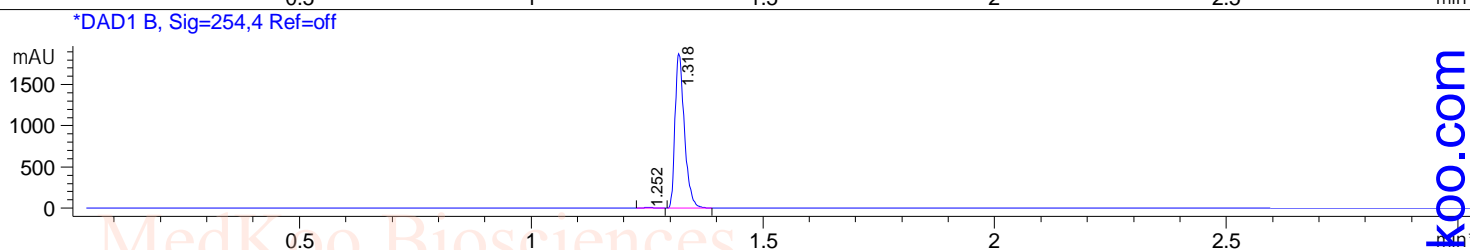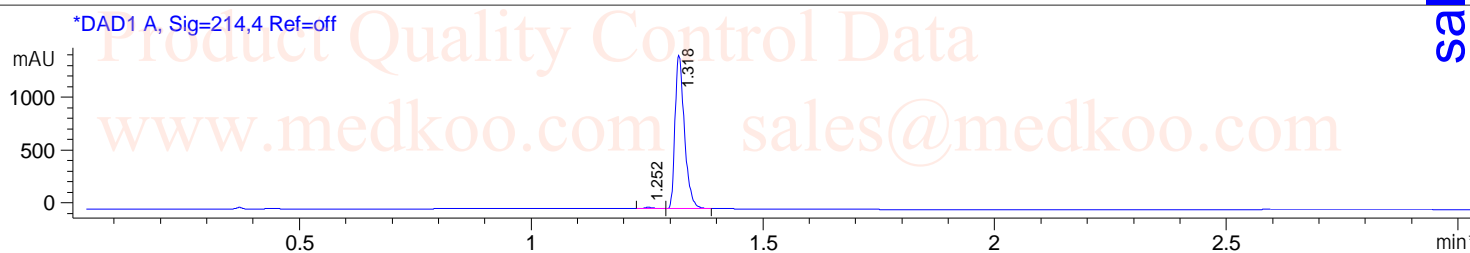

Ret. Time: 1.32

<<<< POSITIVE SPECTRA >>>>

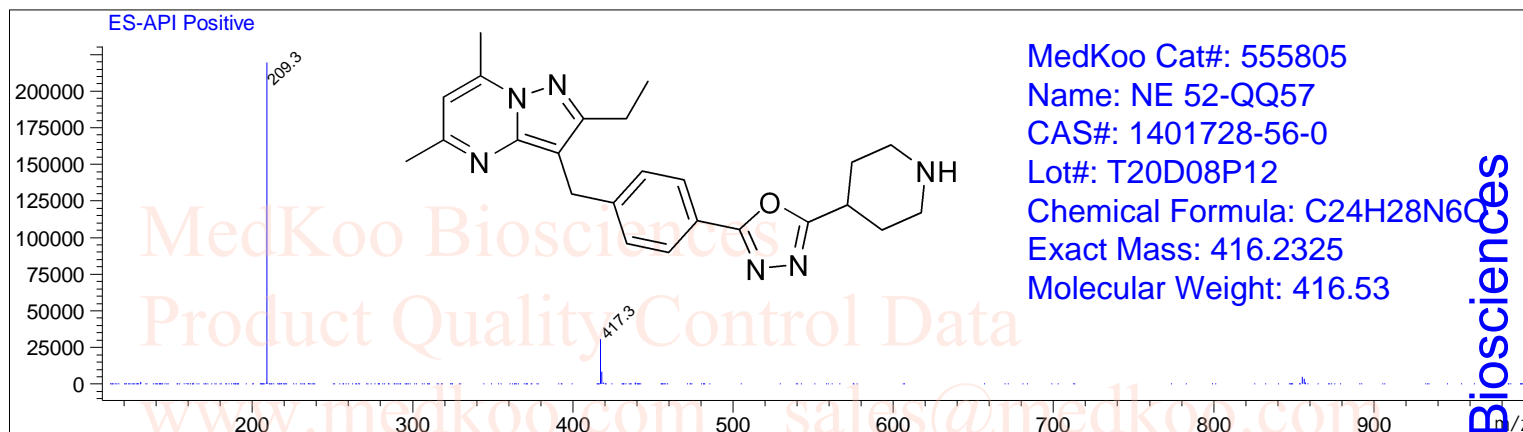

sales@medkoo.com

www.medkoo.com

MedKoo Biosciences